




BEFORE CytoDiff* IMPLEMENTATION, ALL SAMPLES WITH
FLAGS FOR WBC ABNORMALITIES UNDERGO **MANUAL REVIEW**



Move healthcare forward.

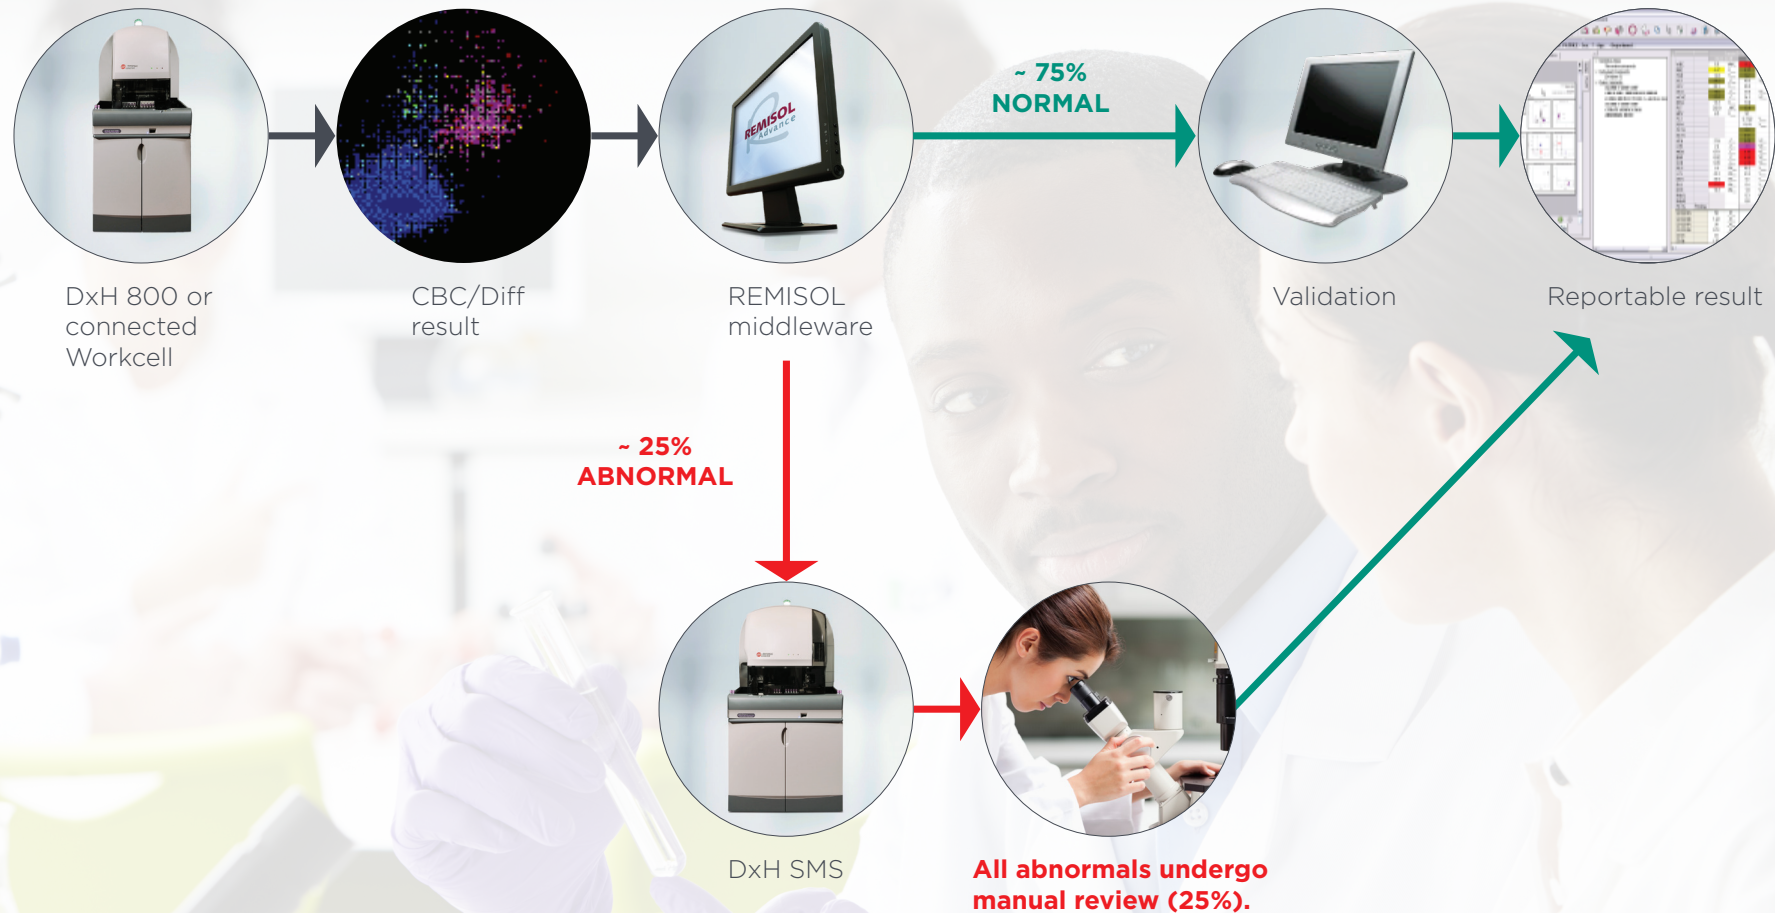


» AFTER CytoDiff* IMPLEMENTATION, 95% OF SAMPLES CAN BE ANALYZED WITH AN **AUTOMATED SYSTEM**



» Move healthcare forward.

Figures and illustration results may vary

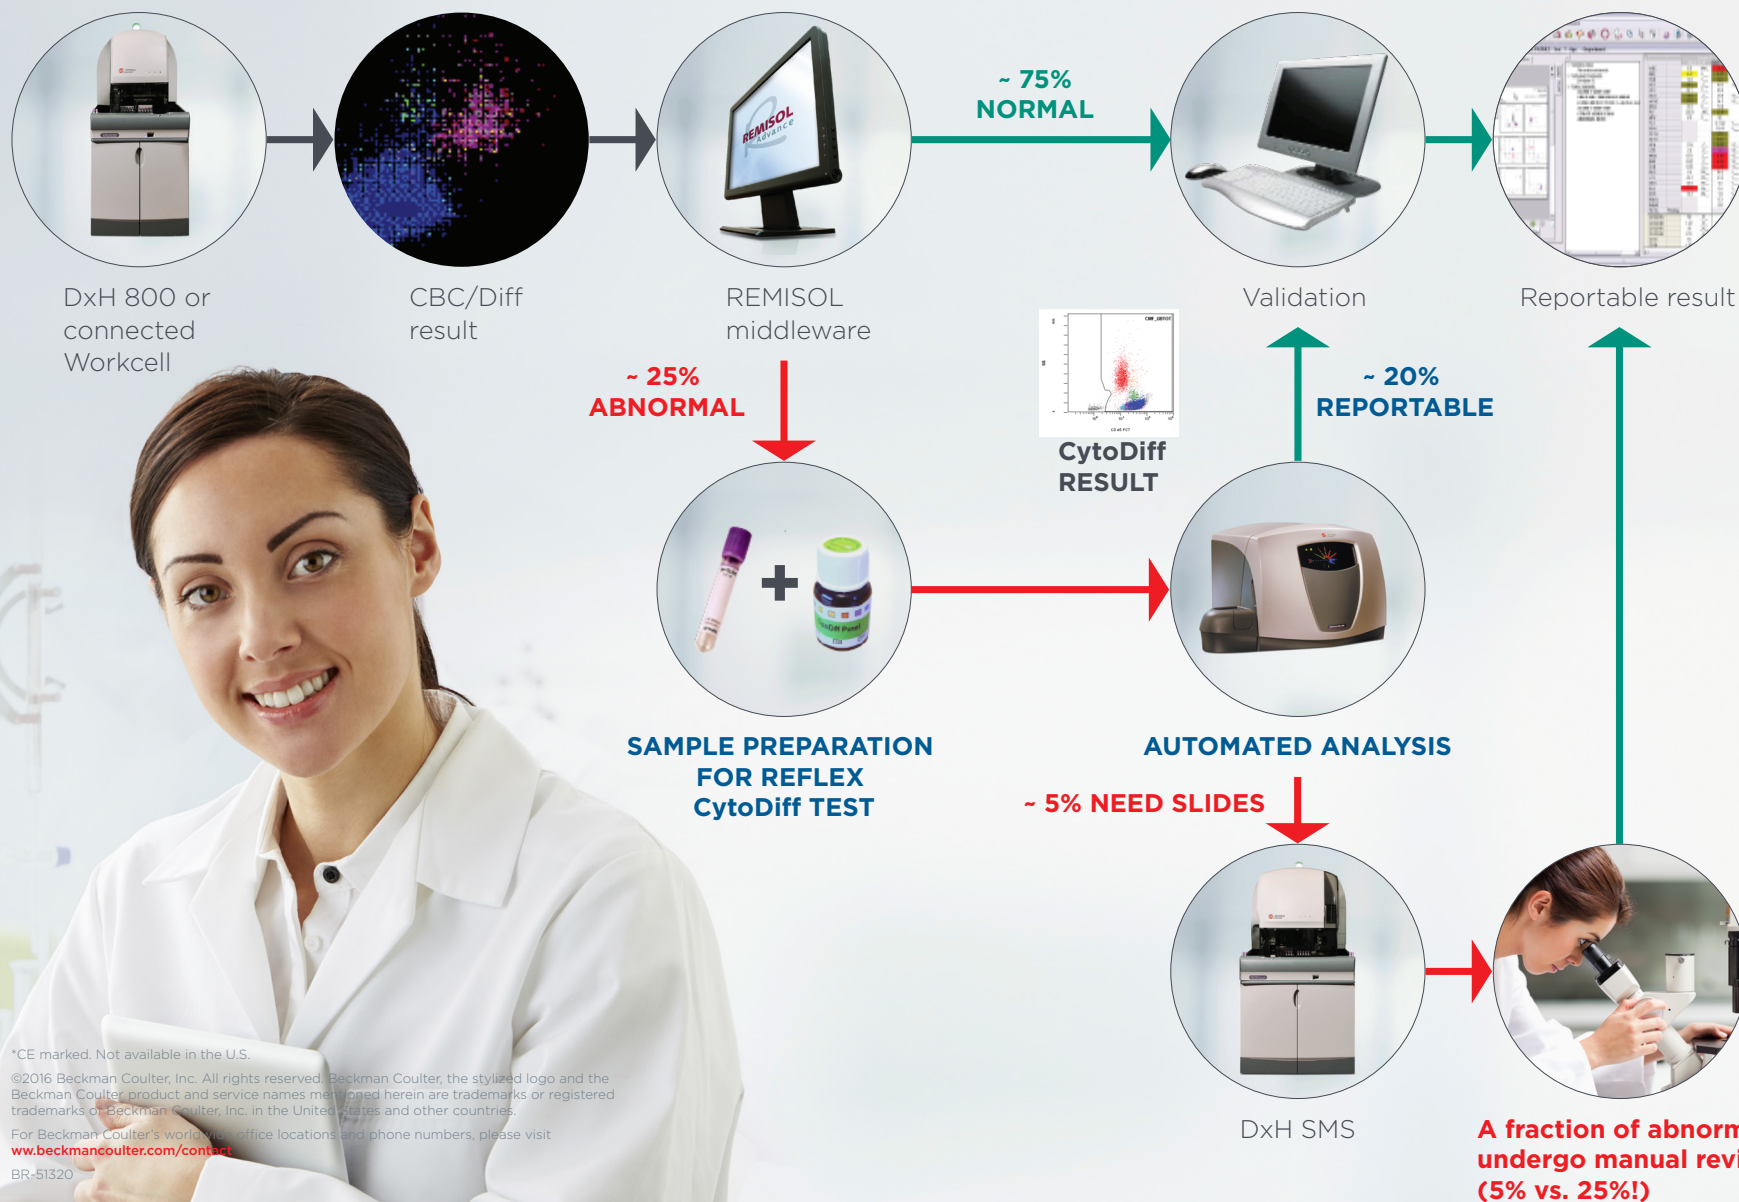

*CE marked. Not available in the U.S.

©2016 Beckman Coulter, Inc. All rights reserved. Beckman Coulter, the stylized logo and the Beckman Coulter product and service names mentioned herein are trademarks or registered trademarks of Beckman Coulter, Inc. in the United States and other countries.

For Beckman Coulter's worldwide office locations and phone numbers, please visit

www.beckmancoulter.com/contact

BR-51320